


Appendixes

Appendix 1: the apparatus:



A-1

coating unit chambers

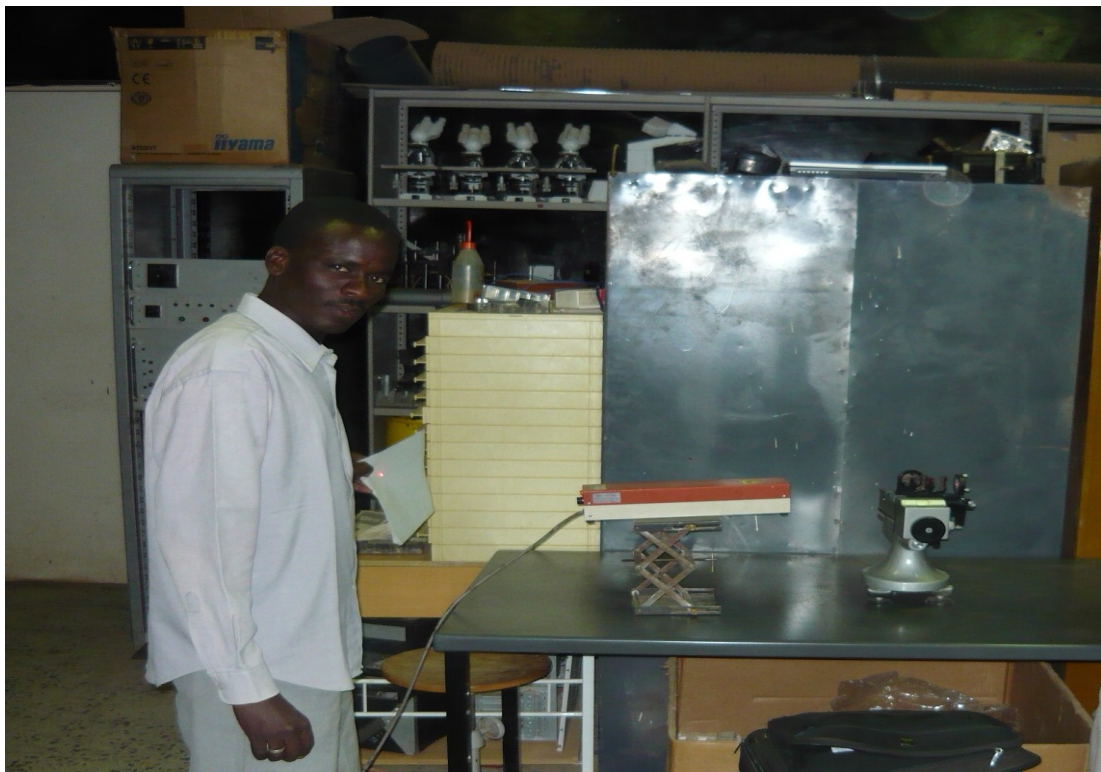




A-2 Michelson interference for thickness measurement




(A-3 Furnace for samples treatment between(50-250 C°


Appendixes 2:


The figures and diagrams of MnS samples:

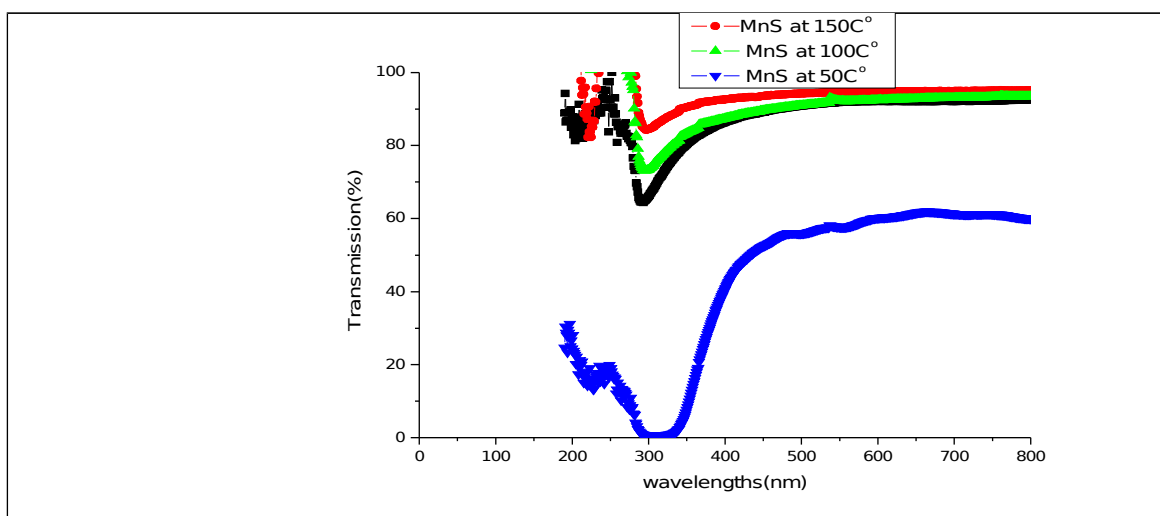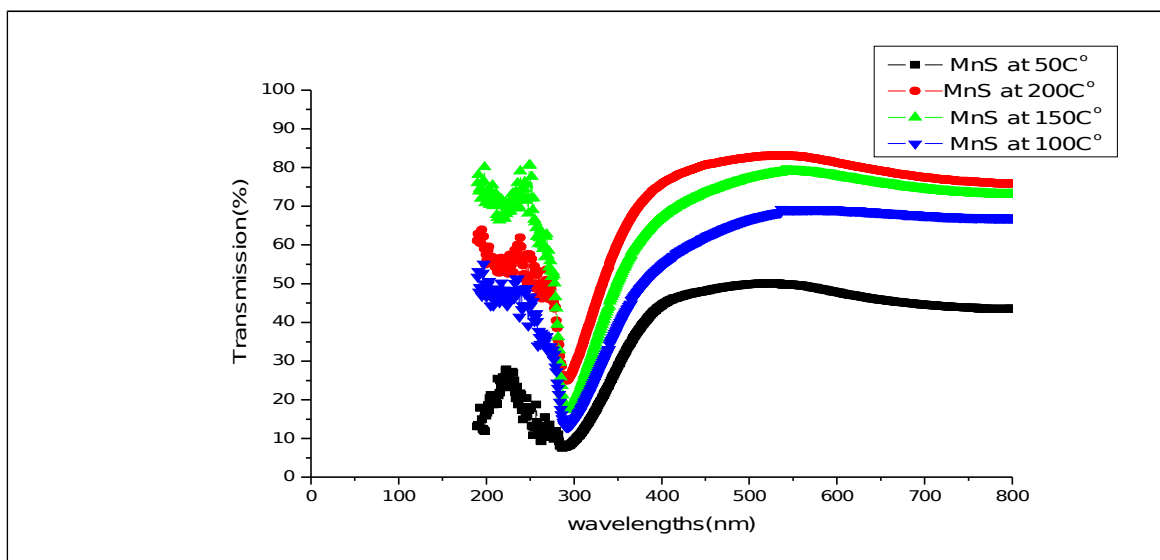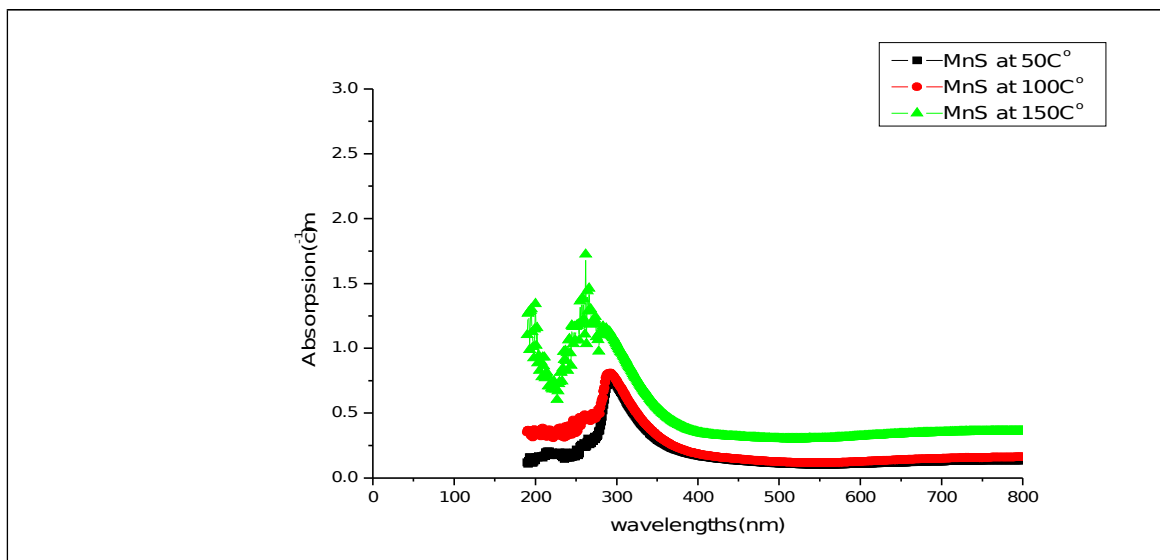

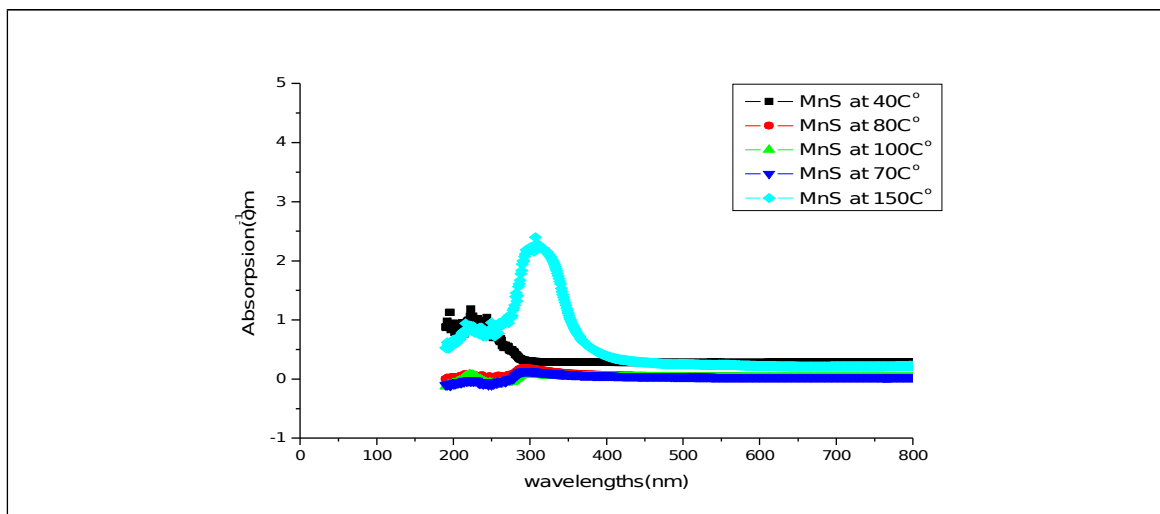


Transmission of *Sample 6*

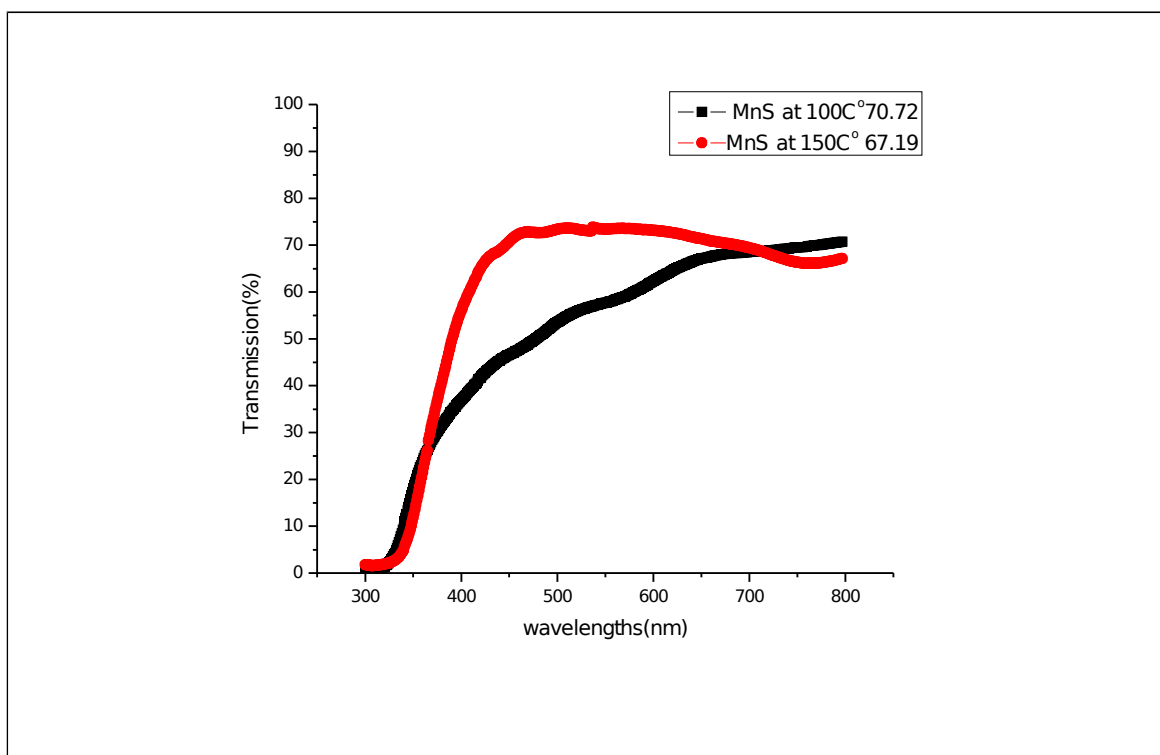


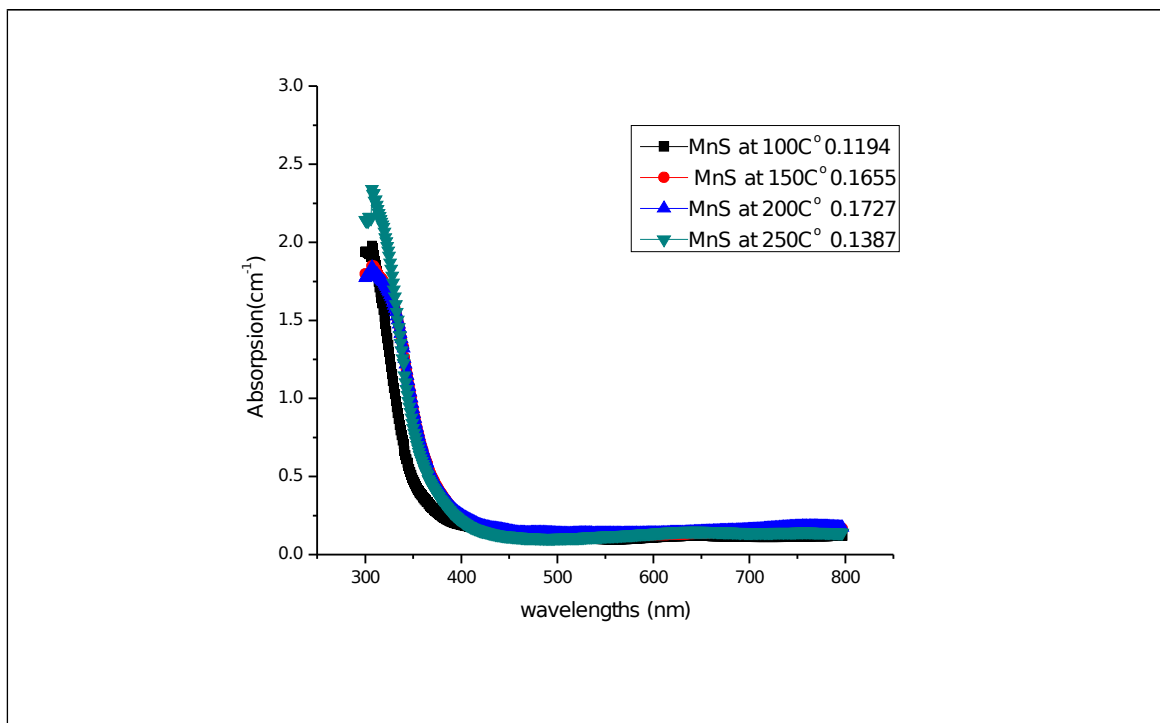


Absorption of Sample 7

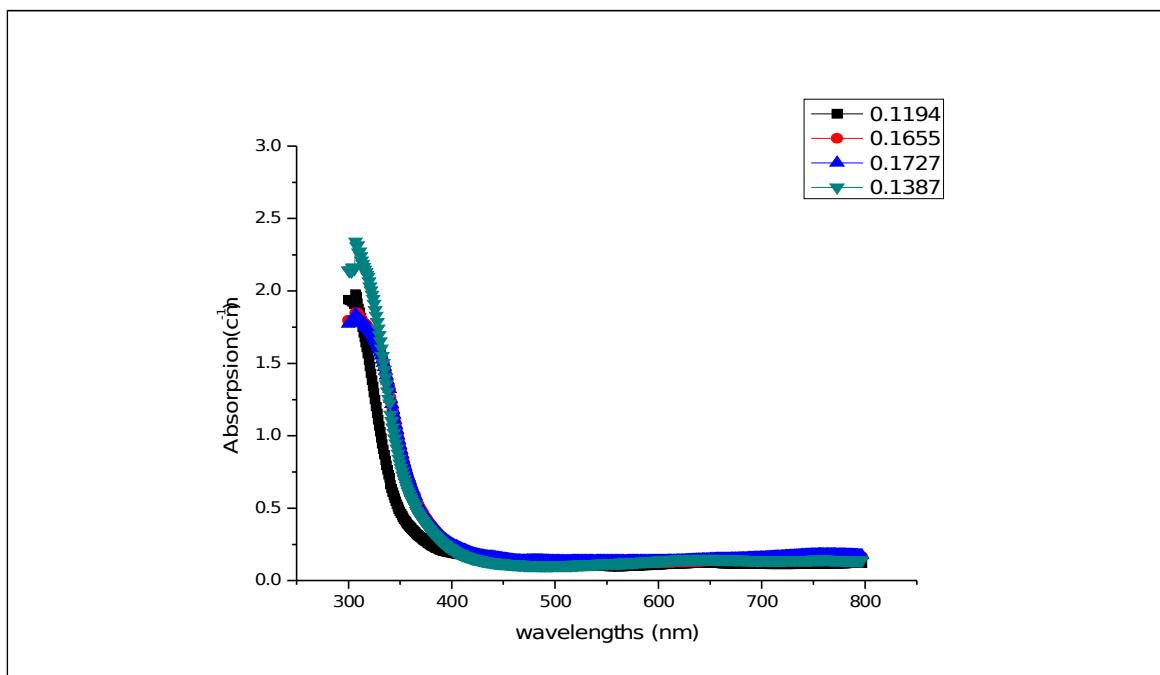

Transmission of sample 7

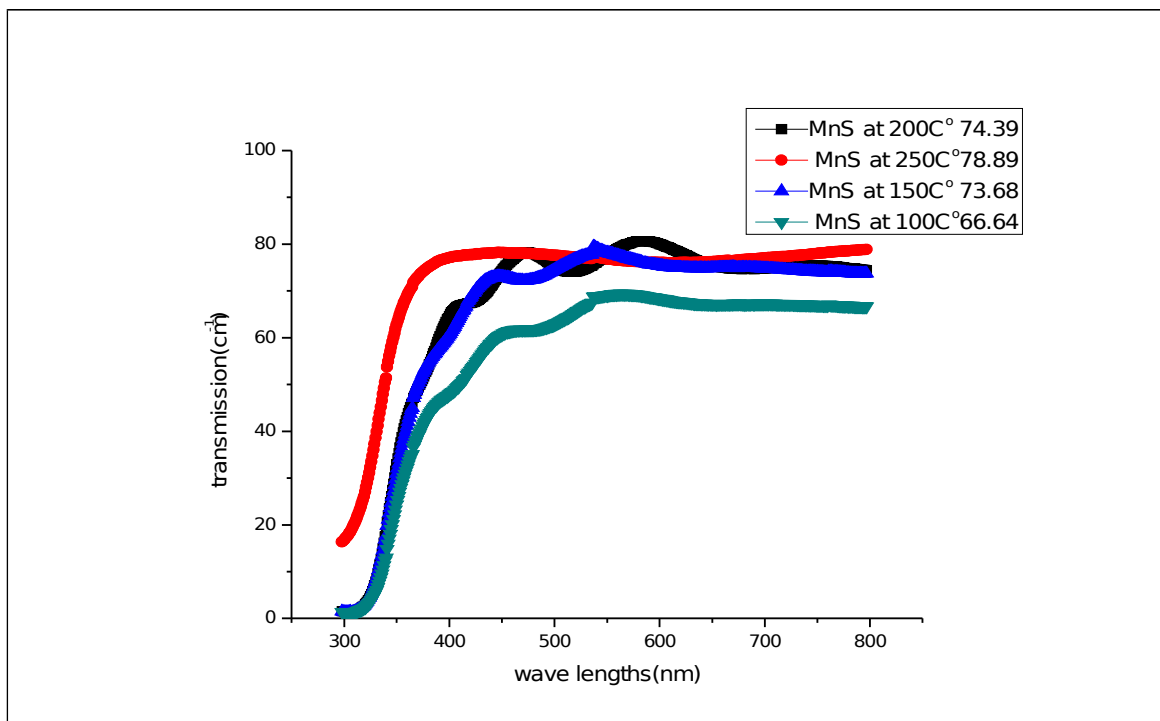

Absorption of sample 5

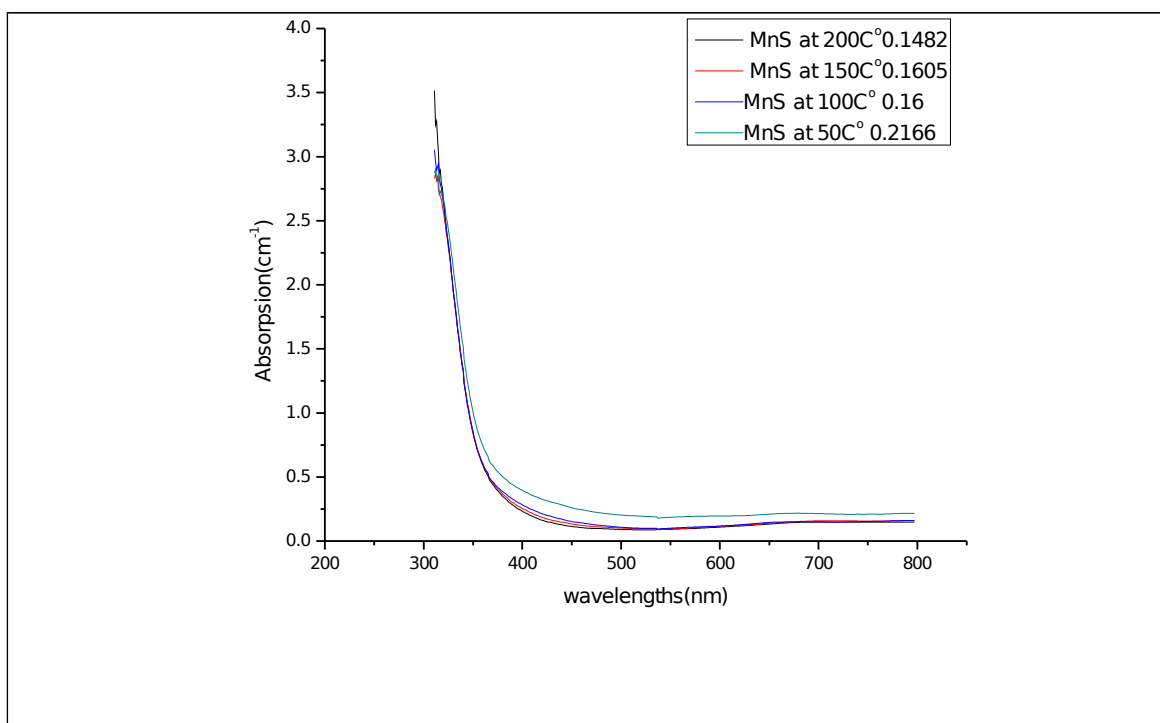

Transmission of sample 5

